

One single-tube PCR assay to detect both CD17 (A>T) and IVS-II nt-654 (C>T) homozygous mutations of β -thalassemia

Qi LIU^{1,*}, Jun-Li WANG^{2,+}, Guo-Can YANG¹, Xue-Jun DONG¹, Zong-Xin WANG¹, Guo-Xing GE¹, Xiao-Feng GU³

¹Shaoxing People's Hospital, Shaoxing Hospital of Zhejiang University, Shaoxing, P.R. China

²Affiliated Hospital of Youjiang Medical University for Nationalities, Baise, P.R. China

³Wenzhou Medical College, Wenzhou, P.R. China

Received: 18.09.2012 • Accepted: 27.11.2012 • Published Online: 26.08.2013 • Printed: 20.09.2013

Aim: Several methods can be used to detect gene mutations associated with β -thalassemia, but it is difficult to achieve reliable and reproducible results. In this study, we introduce a new method, a single-tube multiplex polymerase chain reaction (PCR) assay, to detect both CD17 (A>T) and IVS-II nt-654 (C>T) homozygous mutations.

Materials and methods: This new method designs specific primers to diagnose homozygous mutations and normal controls.

Results: After PCR amplification, homozygous mutations produce different fragments from normal controls.

Conclusion: This study represents an important step towards the development of a novel protocol to diagnose β -thalassemia and other diseases that target numerous mutations.

Key words: β -Thalassemia, single-tube, CD17, IVS-II nt-654

1. Introduction

β -Thalassemia (β -thal) is a severe disorder of β -globin gene expression characterized by hypochromic, hemolytic anemia and inherited as an autosomal disorder (1,2). In general, each ethnic group appears to carry its own profile of mutant alleles. Currently, 265 different point mutations (<http://globin.bx.psu.edu>) have been characterized to be associated with β -thal (3–6), 4 of which can account for about 87% of the occurrence of β -thal. In descending frequencies, these 4 mutations are codon CD41/42(-CTTT), IVS-II nt-654 (C>T), CD17 (A>T), and TATA box nt-28 (A>G) (7). In China, β -thal, with carrier frequencies ranging from 0.02% to 4.8%, affects an estimated 20 million people that are predominantly distributed in Guangxi, Guangdong, Hainan, and Yunnan provinces (8). The universality of this disease produces great mental and economic pressure upon society and the patients' families, which no doubt prevents the development of the public health in southern China (9).

The main clinical diagnostic methods of β -thal are polymerase chain reaction-reverse dot blot (PCR-RDB), real-Time PCR, the polymerase chain reaction-amplification refractory mutation system (PCR-ARMS),

restriction fragment length polymorphism (RFLP), antisense oligodeoxynucleotide (ASO), single-strand conformation polymorphism (SSCP), and Gene Chip (10–13). It took us about 8 h to complete the procedure including PCR and RDB. Previously, the PCR method has been proven to be simple, very sensitive, and specific for the routine diagnosis of β -thal mutation. However, it is difficult to achieve reliable and reproducible results in comparison with a single-tube multiplex PCR assay. In this study, a single-tube multiplex PCR assay has been successfully used to diagnose the 2 most widely occurring β -globin gene mutations in China.

2. Materials and methods

2.1. Patients and samples

In total, 40 unrelated patients (19 females and 21 males, mean age of 40.5 ± 12.9 years) and 20 control patients (12 females and 8 males, mean age of 41.3 ± 6.8 years) were investigated in this study. All patients had no other diseases. All individuals enrolled gave informed written consent as approved by the local institutional review board. The investigated mutations included 20 CD17 (A>T) homozygous mutations and 20 IVS-II-654 (C>T)

* Correspondence: jokaing@163.com

+ These authors contributed equally to this work.

homozygous mutations. Genomic DNA was isolated from whole blood of participants using the Puregene DNA Isolation Kit (QIAGEN, Hong Kong).

2.2. Primer designs

Giving the detection of the CD17 (A>T) homozygous mutation for an example, we carried out a parallel multiplex PCR reaction by using a pair of primers, 5'-ATTGCTTACATTTGCTTCTG-3' and 5'-ACTTCATCCACGTTCAGCTT-3', for the specific amplification of the CD17A and CD17T alleles, respectively (128-bp fragments; Table 1). The reverse primer differs only in the mutated nucleotide at its 3' end. We in let a C>G change (the modified nucleotide is underlined), which will cause an additional mismatch to increase the allele specificity of the reaction, shorten the annealing temperature, and rule out the nonspecific PCR amplification. The specific mismatch site could provide a relatively large difference of melting temperature. We also introduced another pair of primers, 5'-TGATAATTTCTGGGTTATGGT-3' and 5'-AATATCCCCCAGTTTAGTAG-3', for the detection of the IVS-II-654 (C>T) homozygous mutation (Table 1). GeneTool (GeneBio, Switzerland) software was used to design the primers.

2.3. PCR reaction

PCR reaction was carried out in a Bio-Rad S1000 PCR System (Bio-Rad Laboratories, USA) with 1 cycle of denaturation at 95 °C for 5 min; 5 touch-down cycles of denaturation at 94 °C for 40 s, annealing for 40 s at 53 °C for the first cycle, and a 1 °C reduction per cycle; 25 cycles of denaturation at 94 °C for 40 s and annealing at 48

°C for 40 s; and a final extension step at 72 °C for 7 min. The reaction was carried out in a final volume of 50 µL at the same concentration of 4 primers for CD17 (A>T) and IVS-II-654 (C>T) homozygous mutations, with a final concentration of 1 or 2.5 mM magnesium chloride and 100 ng of DNA template, using Taq DNA polymerase (TaKaRa, China). PCR products were separated by agarose gel electrophoresis (2.0% agarose gel; Figure 1) and visualized using Bio-Rad Chemi Doc XRS (Bio-Rad Laboratories). Fragment size was determined by comparison to a 2-kb DNA marker (Invitrogen, USA). DNA sequencing of the β-globin gene was performed using 2 pairs of primers flanking the 3 exons of β-globin genes, and DNA was amplified using Taq DNA polymerase (TaKaRa) in the Bio-Rad S1000 PCR System (Bio-Rad Laboratories). The primers and product lengths are shown in Table 2. The PCR product was sequenced using the ABI3700 (ABI, USA) and visualized using the Chromas program.

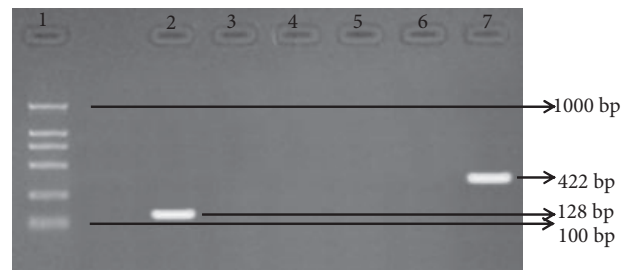


Figure 1. One specific single-tube polymerase chain reaction for both CD17 (A>T) and IVS-II-654 (C>T) homozygous mutations. Lane 1 was 2-kb DNA marker; 2 was CD17T-specific PCR; 7 was IVS-II-654T-specific PCR; 3, 4, 5, and 6 were normal controls.

Table 1. PCR primer sequences, fragment sizes, and gene location.

| ID | Primer sequence (5'-3') | Fragment size (bp) | GenBank No. : nucleotides |
|------|-------------------------------|--------------------|---------------------------|
| No.1 | ATTGCTTACATTTGCTTCTG | 128 | NG_000007 : 70538-70557 |
| No.2 | ACTTCATCCACGTT <u>CAGCTT</u> | | NG_000007 : 70646-70665 |
| No.3 | TGATAATTTCTGGGTTA <u>TGGT</u> | 422 | NG_000007 : 71673-71693 |
| No.4 | AATATCCCCCAGTTTAGTAG | | NG_000007 : 72075-72094 |

Table 2. β-Globin primers for PCR and sequencing.

| Gene | Primer sequence (5'-3') | Fragment size (bp) | GenBank No. : nucleotides |
|--------------|-------------------------------------|--------------------|---------------------------|
| β1 (exon1-2) | Forward: GTACGGCTGTCATCACTTAGACCTCA | 602 | NG_000007 : 70416-70441 |
| | Reverse: TGCAGCTTGTCACAGTGCAGCTCACT | | NG_000007 : 70992-71017 |
| β2 (exon3) | Forward: GTGTACACATATTGACCAAA | 423 | NG_000007 : 71496-71515 |
| | Reverse: AGCACACAGACCAGCACGTT | | NG_000007 : 71899-71918 |

3. Results

The electrophoresis results showed that the single-tube multiplex PCR assay worked well (Figure 2). CD17 (A>T) and IVS-II-654 (C>T) homozygous mutations could be detected in a single tube. After amplification, the CD17 (A>T) samples could produce a 128-bp fragment with the combination of 4 primers. Meanwhile, the IVS-II-654 (C>T) samples could produce a 422-bp fragment with the combination of 4 primers. However, the normal control samples produced no fragment using the combination of 4 primers. In a verification test, all samples that had been detected by DNA sequencing were analyzed by single-tube PCR assay, and the results showed complete agreement between the new method and sequencing analysis. To evaluate the reproducibility of the single-tube PCR assay, all samples were tested 5 times, and all the mutant and wild-type blots showed the same depth of color every time. Heterozygous samples were excluded since this method was a qualitative analysis and could not discriminate between heterozygous samples and homozygous samples. For detecting more homozygous mutations in future studies, reducing the requirements of multiple reaction conditions in a single tube, we did not use internal control in this PCR assay, but negative nontemplate controls were included in each PCR. PCR products were subjected to electrophoresis on agarose gels and sequenced.

4. Discussion

Although β -thal is a genetic disease that has been well characterized at the DNA level, mutation detection in the β -globin gene is still based on time-consuming methodologies, requiring cumbersome sample manipulation. Commonly, the occurring mutations of the β -globin gene are detected by a number of PCR-based procedures, such as RDB analysis or primer-specific amplification with a set of probes (10,13). Other methods based on real-time PCR or microarray technology (11,12) are incompatible for the routine clinical laboratory because of their cost and complexity.

In view of the above drawbacks, in this study, we have explored a different approach based on specific primers. It is indicated that single-tube multiplex PCR assay could quickly and simply detect both CD17 (A>T) and IVS-II-654 (C>T) homozygous mutations. The frequency of CD17 (A>T) and IVS-II-654 (C>T) mutations in China is 0.10%–1.59% and 0.57%–0.63%, respectively (14,15). We found that this method is less laborious, less expensive, and faster, which makes it more suitable for routine diagnosis. Therefore, this method can be well extended to detect other gene mutations.

It should also be noted that the single-tube multiplex PCR assay has some limitations. For example, we can only detect 2 homozygous mutations in a single tube; a heterozygous mutation (a mutation of only 1 allele) and

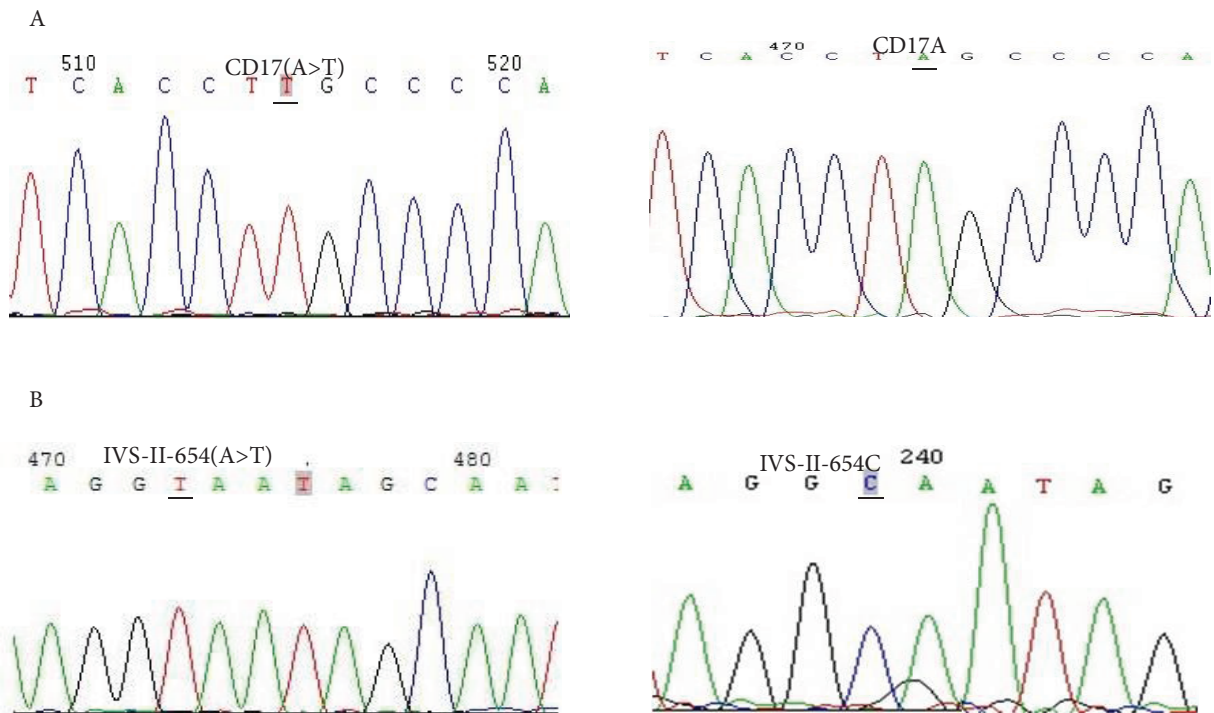


Figure 2. Sequencing results of (A) homozygous CD17 (A>T) mutation and wild type, (B) homozygous IVS-II-654 (C>T) mutation and wild type.

compound heterozygous mutations (2 different mutations in the paternal and maternal alleles) could not be detected at present. However, we expect that this method will be perfected with continuous improvement of various analytical techniques.

In summary, this study represents an important step toward the development of a novel protocol to diagnose β -thal and other diseases that target numerous mutations.

References

1. Bunn HF, Forger BG. Hemoglobin: Molecular, Genetic and Clinical Aspects, 1st ed. Philadelphia: WB Saunders; 1986.
2. Batebi A, Pourreza A, Esmailian R. Discrimination of beta-thalassemia minor and iron deficiency anemia by screening test for red blood cell indices. *Turk J Med Sci* 2012; 42: 275–80.
3. Orkin SH, Kazazian HH Jr. The mutation and polymorphism of the human beta-globin gene and its surrounding DNA. *Annu Rev Genet* 1984; 18: 131–71.
4. Antonarakis SE, Irkin SH, Cheng TC, Scott AF, Sexton JP, Trusko SP et al. β -Thalassemia in American Blacks: novel mutations in the “TATA” box and an acceptor splice site. *Proc Natl Acad Sci USA* 1984; 81: 1154–8.
5. Kazazian HH Jr, Orkin SH, Antonarakis SE, Sexton JP, Boehm CD, Goff SC et al. Molecular characterization of seven beta-thalassemia mutations in Asian Indians. *EMBO J* 1984; 3: 593–6.
6. Cheng TC, Orkin SH, Antonarakis SE, Potter MJ, Sexton JP, Markham AF et al. β -Thalassemia in Chinese: use of in vivo RNA analysis and oligonucleotide hybridization in systematic characterization of molecular defects. *Proc Natl Acad Sci USA* 1984; 81: 2821–5.
7. Chan V, Chan TK, Chebab FF, Todd D. Distribution of beta-thalassemia mutations in south China and their association with haplotypes. *Am J Hum Genet* 1987; 41: 678–85.
8. Xu XM, Zhou YQ, Luo GX, Liao C, Zhou M, Chen PY et al. The prevalence and spectrum of alpha and beta thalassaemia in Guangdong Province: implications for the future health burden and population screening. *J Clin Pathol* 2004; 57: 517–22.
9. Lin M, Zhu JJ, Wang Q, Xie LX, Lu M, Wang JL et al. Development and evaluation of a reverse dot blot assay for the simultaneous detection of common alpha and beta thalassemia in Chinese. *Blood Cells Mol Dis* 2012; 48: 86–90.
10. Cao A, Galanello R. Beta-thalassemia. *Genet Med* 2010; 12: 61–76.
11. Vrettou C, Traeger-Synodinos J, Tzetzis M, Malamis G, Kanavakis E. Rapid screening of multiple beta-globin gene mutations by real-time PCR on the LightCycler: application to carrier screening and prenatal diagnosis of thalassemia syndromes. *Clin Chem* 2003; 49: 769–76.
12. Ye BC, Zhang Z, Lei Z. Molecular analysis of alpha/beta-thalassemia in a southern Chinese population. *Genet Test* 2007; 11: 75–83.
13. Clark BE, Thein SL. Molecular diagnosis of haemoglobin disorders. *Clin Lab Haematol* 2004; 26: 159–76.
14. Xiong F, Sun M, Zhang X, Cai R, Zhou Y, Lou J et al. Molecular epidemiological survey of haemoglobinopathies in the Guangxi Zhuang Autonomous Region of southern China. *Clin Genet* 2010; 78: 139–48.
15. Xu XM, Zhou YQ, Luo GX, Liao C, Zhou M, Chen PY et al. The prevalence and spectrum of α - and β -thalassemia in Guangdong Province: implications for the future health burden and population screening. *J Clin Pathol* 2004; 57: 517–22.

Acknowledgments

We thank Dr Min Fang for providing language help and writing assistance. This study was supported by the Foundation of Shaoxing Science and Technology Project (No. 2012B70058). This study was also supported by the National Natural Science Foundation (No. 81161202) and by the Foundation of the Health Department of Guangxi Province, China (No. 2012713, 2012085).